

(19)



Europäisches Patentamt

European Patent Office

Office européen des brevets



(11)

**EP 0 597 967 B1**

(12)

**EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention  
of the grant of the patent:  
**01.12.1999 Bulletin 1999/48**

(21) Application number: **92916897.9**

(22) Date of filing: **15.07.1992**

(51) Int. Cl.<sup>6</sup>: **A61F 2/24**

(86) International application number:  
**PCT/US92/05919**

(87) International publication number:  
**WO 93/01768 (04.02.1993 Gazette 1993/04)**

**(54) DEVICES FOR PERFORMING INTRALUMINAL PROCEDURES**

VORRICHTUNGEN ZUR DURCHFÜHRUNG INTRALUMINALER EINGRIFFE

APPAREILS UTILISABLES POUR DES PROCEDES DANS UN CONDUIT CORPOREL

(84) Designated Contracting States:  
**CH DE ES FR GB IT LI**

(30) Priority: **16.07.1991 US 730559**

(43) Date of publication of application:  
**25.05.1994 Bulletin 1994/21**

(60) Divisional application:  
**99108298.3 / 0 937 439**

(73) Proprietor: **HEARTPORT, INC.**  
**Redwood City, CA 94063 (US)**

(72) Inventor: **STEVENS, John H.**  
**Palo Alto, CA 94303 (US)**

(74) Representative:  
**Harrison, David Christopher et al**  
**MEWBURN ELLIS**  
**York House**  
**23 Kingsway**  
**London WC2B 6HP (GB)**

(56) References cited:

<b>WO-A-91/17720</b>	<b>US-A- 3 409 013</b>
<b>US-A- 3 540 431</b>	<b>US-A- 3 587 115</b>
<b>US-A- 3 787 899</b>	<b>US-A- 4 056 854</b>
<b>US-A- 4 574 803</b>	<b>US-A- 4 612 011</b>
<b>US-A- 5 069 015</b>	<b>US-E- R E33 258</b>

Note: Within nine months from the publication of the mention of the grant of the European patent, any person may give notice to the European Patent Office of opposition to the European patent granted. Notice of opposition shall be filed in a written reasoned statement. It shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

**EP 0 597 967 B1**

## Description

[0001] This invention relates to devices for performing an intraluminal procedure and in particular to devices for endovascular replacement of a heart valve.

[0002] It is often necessary to replace malfunctioning heart valves within the body. Heart valve replacement generally has been accomplished by a major open heart surgical procedure, requiring general anesthesia, full cardiopulmonary bypass with complete cessation of cardiopulmonary activity, seven to ten days of hospitalization and months of recuperation time. The mortality rate with this type of procedure is about five to six percent.

[0003] Endovascular procedures for valve replacement provide an alternative to open heart surgery. For example, in patients with serious aortic valve disease who are too compromised to tolerate open heart surgery, surgeons have used endovascular balloon aortic valvuloplasty. This procedure involves use of endovascular balloon dilatation to split commissures in diseased aortic valves with commissural fusion and to crack calcific plaques in calcified stenotic aortic valves. This method provides only partial and temporary relief for a patient with a stenotic aortic valve. A repeat procedure within a year of the first procedure is often required.

[0004] An alternative treatment regimen is endovascular valve substitution. In this procedure, instruments are used to insert a mechanical valve in the lumen of a central blood vessel via entry through a distal artery, for example, the brachial or femoral artery. The descriptive terms distal and proximal, when used in relation to the vasculature in this application, refer to directions further and closer from the valve replacement or procedure site, as applicable. A guide wire is placed through the entry vessel and fluoroscopically directed to the desired situs. Flexible catheters are then guided over the guide wires which are used to propel and direct the new valve through the blood vessel to the desired central location near to the malfunctioning heart valve where it supplants the function of the existing valve.

[0005] Endovascular heart procedures, in contrast to open heart surgical procedures, would require only local anesthesia, partial or no cardiac bypass, one to two days hospitalization, and should have a reduced mortality rate as compared to open heart procedures. However, as discussed in the literature but never actually practiced, endovascular heart valve substitution is limited to supra-annular arterial based mechanical valves which require an elongated mounting catheter originating at the distal arterial entry point to maintain the position of the valve in the aorta and therefore does not provide a permanent or internalized system. Valve substitution is also limited to treating regurgitant aortic valves and is not applicable to stenotic aortic valves or any other malfunctioning heart valves. In addition, once implanted, mechanical valves predispose the patient to thrombus formation and emboli, mandating long term

anticoagulant therapy; intracranial hemorrhages are a serious side effect of long term anticoagulant therapy.

[0006] A potential alternative to a mechanical valve is a bioprosthetic valve. A bioprosthetic valve can be either a homograft (a fresh human), allograft (a fixed human) or a xenograft (a fixed other species) valve. Homograft valves, in contrast to xenograft valves, are rarely used because of the lack of access to fresh human valves. Porcine glutaraldehyde preserved valves are often used since they are readily accessible and storable and are available in a variety of sizes. Bioprosthetic valve replacement does not predispose a patient to thrombus formation or emboli, and, therefore, requires no long-term anticoagulant therapy. Bioprosthetic valves are presently a mainstay in aortic valve replacement. Bioprosthetic heart valve replacement is preferable in patients who cannot tolerate long-term anticoagulant therapy or are otherwise potentially noncompliant with a long term medical regime.

[0007] To date, bioprosthetic and mechanical valves have been inserted near or at the native annulus site through open heart surgery and except for the Magovern-Cromie Valve which used pins to fix the valves have required sutures for fixation at the insertion site; means for endovascular valve replacement with any valve are not available. It would therefore be of interest to provide a endovascular means i) to easily remove a dysfunctional natural or prosthetic valve and ii) to replace the dysfunctional valve with a endovascularly replaceable bioprosthetic or flexible synthetic valve, independently fixed without sutures or catheter, near or at the native valve annulus site.

[0008] US-A- 3,671,979 to Mouloupoulos, issued June 27, 1972, describes a endovascularly inserted conical shaped umbrella-like valve positioned and held in place by an elongated mounting catheter at a supra-annular site to the aortic valve in a nearby arterial vessel. The conical end points toward the malfunctioning aortic valve and the umbrella's distal ends open up against the aorta wall with reverse blood flow, thereby preventing regurgitation.

[0009] US-A- 4,056,854 to Boretos, issued November 8, 1977, describes a endovascularly inserted, catheter mounted, supra-annular valve delivered while constrained in a capsule, the circular frame of the valve expanding to abut the wall of the artery and attached flaps of flexible membrane extend distally in the vasculature once free of the delivery capsule. The flaps lie against the artery wall during forward flow, and close inward towards the central catheter to prevent regurgitation during reverse blood flow. The Boretos valve was designed to be positioned against the artery wall during forward flow, as compared to the mid-center position of the Mouloupoulos valve, to reduce the stagnation of blood flow and consequent thrombus and embolic formation expected from a valve at mid-center position.

[0010] Reviews relating to replacement valves include: *Gibbon's Surgery of the Chest*, 5th Ed., David

C. Sabiston, Jr., M.D., Frank D. Spencer, M.D., 1990, Vol. II, Ch. 52, pp. 1566-1596, and Textbook of Interventional Cardiology, Eric J. Topol, 1990, Chs. 43-44, pp. 831-867.

[0011] In contrast to US-A-4056854, according to a first aspect of the invention, a delivery capsule for a replacement valve has a bracer to hold the capsule in position while the valve is forced from it.

[0012] Preferably, said bracer is circumferentially differentially expandable for holding said introducer capsule in position during delivery of said replacement valve device.

[0013] Preferably, said pusher is a disc.

[0014] US-A-4,787,899 discloses a system for performing an intraluminal procedure, in particular an intraluminal grafting system.

[0015] US-A-3540431 shows a barrier for a lumen of the body which is delivered endoluminally by constraint within a capsule. It is attached to a guide wire by which it can be moved out of the capsule, so that it expands into contact with the lumen.

[0016] A barrier according to a second aspect of the present invention, however, has a circumferentially differentially expandable bracer which allows changes in the angle of a working channel of the barrier in relation to the situs.

[0017] Preferably, the barrier is of selectively permeable material with a distal end configured to point downstream in the host.

[0018] There may be a tissue cutter for removal of undesired tissue, the tissue cutter having at least one blade and a cable, said at least one blade being movable to an unextended condition and being capable of endovascular passage to the situs while in that condition.

[0019] Preferably, said at least one blade has a hinge for allowing movement of the blade to and from the extended and unextended conditions.

[0020] Embodiments of the present invention will now be described by way of example only with reference to the accompanying drawings, in which:

Figure 1 illustrates a procedure device capsule side view.

Figure 2 illustrates a side view of an intraluminal procedure device.

Figure 3 illustrates a bottom view of an intraluminal procedure device.

Figure 4 illustrates a top view of an intraluminal procedure device.

Figure 5 illustrates a tissue cutter in a closed position.

Figure 6 illustrates a tissue cutter in an open position.

Figure 7 illustrates a side view of a valve introducer capsule with bracer balloons deflated.

Figure 8 illustrates a side view of a valve introducer capsule with bracer balloons inflated.

Figure 9 illustrates a side view of a valve introducer capsule with balloons passed over a guide wire.

Figure 10 illustrates a side view of a pusher disc advancing a valve out of the introducer capsule.

Figure 11 illustrates an aortic valve in the side position.

Figure 12 illustrates an aortic valve from the top view.

Figure 13 illustrates a side view of an aortic valve with the mounting ring in the closed position.

Figure 14 illustrates a front view of an aortic valve with the mounting ring in the open position.

Figure 15 is a graphic illustration of a side view of a mounting pin confirmation change with balloon inflation.

[0021] The present invention, in a preferred aspect relates to devices for the (supplantation or) replacement of a cardiac valve in a host through endovascular means. The valve replacement system includes up to five devices: (1) a prosthetic valve device, (2) a valve introducer device, (3) an intraluminal procedure device, (4) a procedure device capsule, and (5) a tissue cutter. Not all the devices of the system are required to be used as they are for valve replacement; the description of valve replacement using all the components is merely exemplary.

[0022] In a general method, the procedure device capsule (Fig. 1), which contains the intraluminal procedure device, is inserted into an entry point in the host and used to transport the intraluminal device to the desired situs, over a guide wire. At the situs, a selectively permeable barrier of the intraluminal procedure device exits from the procedure device capsule, expands in a controlled and adjustable manner and abuts the lumen of the vessel encircling the old valve or prosthesis (Figs. 2, 3 & 4). The guide wire is withdrawn from the working channel of the intraluminal procedure device leaving the channel available for the passage of the tissue cutter, angioscope, ultrasound, tissue graspers, and tissue cutting devices. The channel can also be used for irrigation or applied to suction apparatus to remove debris, thrombus or other material.

[0023] The tissue cutter then is inserted into the host through the working channel of the intraluminal procedure device to the valve situs where it is used to cut and remove the existing valve from the situs (Figs. 5, 6). Accurate positioning of the cutter is assured using transesophageal echocardiography and intra-arterial or intra-cardiac ultrasound and angiography. The precision of the valve extraction and replacement is important to the success of endovascular valve replacement. There are several imaging techniques presently available providing complementary options to assure this precision: 1) Transesophageal echocardiography can be continuously used; 2) Intravascular ultrasound passed through the working channel of the intraluminal procedure device; 3) Intravascular ultrasound passed intravascu-

larly via the venous system through the intraatrial septum across the mitral valve and into the left ventricle; 4) An angioscope can be passed into the left ventricle in a like manner which would provide the added benefit of allowing constant high definition imaging of the entire procedure and high flow irrigation.

[0024] Any tissue debris resulting from the procedure is trapped by the barrier of the intraluminal procedure device or is removed from the host through suction and tissue retrieval devices inserted via the working channel of the intraluminal procedure device. Tissue debris is removed via the working channel of the intraluminal procedure device with suction, grasping devices (e.g. dorrer basket or grasping forceps) or is caught in the barrier of the intraluminal procedure device to avoid embolism. Once all the necessary tissue has been removed, contraction of the tissue cutter allows for removal of the tissue cutter through the working channel of the intraluminal procedure device. The barrier of the intraluminal procedure device is contracted and the intraluminal procedure device is withdrawn into the procedure device capsule which is then removed.

[0025] The valve introducer device containing the prosthetic valve device is then inserted and used to transport the replacement valve to the valve situs, over a guide wire (Fig. 7). The bracer of the valve introducer device, which optionally can include positioning balloons surrounding the introducer capsule of the valve introducer device, inflates in a differential manner, such that certain balloons inflate more or less than others, to assure accurate positioning of the prosthetic valve when delivered out of the introducer capsule (Fig. 8). A means for pushing the valve out of the introducer capsule, after the introducer capsule is in the appropriate position, is to advance the pusher device of the valve introducer device within the capsule (Fig. 9). A means for securing the mounting pins into the desired situs is to inflate a balloon inside of the prosthetic valve device and within the lumen of the mounting ring (Figs. 10-15). The capsule positioning balloons and the intraluminal balloon can then be deflated and the valve introducer device is withdrawn.

[0026] In order to support the circulation of the patient during the endovascular aortic valve replacement it will be necessary to place the patient on partial or complete cardiopulmonary bypass. There are presently available several means to provide this support. For example, one method is percutaneous insertion of venous and arterial cannula with decompression of the left ventricle by insertion of a pulmonary arterial line allowing aspiration of blood and marked diminution of left ventricular filling and ejection.

[0027] The invention provides several advantages, including the ability to replace or supplant existing cardiac or other valves or prostheses via a sutureless endovascular means avoiding the riskier, more expensive and complicated open heart surgical procedure. This prosthetic valve device, preferably using a biopro-

thesis or other thrombus resistant flexible prosthesis for the valve leaflets, will avoid the need for permanent anticoagulant therapy for the host. Once inserted, the valve is capable of operating autonomously. Further, bioprosthesis replacement valves in the past have required sutures and, therefore, open heart surgery for fixation at the annulus or vasculature situs. The mounting device used with the valve allows it to be fixed via endovascular means without the need for sutures. The prosthetic valve device is inserted on a permanent basis, and remains for the life of the valve incorporated in the device. The life of a bioprosthetic valve, for example, can extend to over twenty years. Future developments can provide alternative prosthetic valves with a markedly extended life. Since most of the patients who are unable to tolerate open heart procedures are elderly, the bioprosthetic valve will usually outlive the patient. The intraluminal procedure device and the cutter allow for the novel ability to perform endovascular procedures without the serious side effect of causing loose debris and other emboli to circulate within the vasculature.

[0028] The components of the valve replacement system will now be described. The procedure device capsule comprises a cylindrical sleeve made of flexible durable material, for example, teflon coated polyurethane or other materials which have the following characteristics: flexible such that it can be maneuvered easily through vasculature, durable such that it can withstand the abrasive contact and pressure of instruments inserted and contained within it, and non-thrombogenic such that blood clots do not develop and adhere to its surface. The procedure device capsule has a generally cylindrical outside surface and a generally cylindrical inside surface with a mesh or grid design. It is characterized as capable of containing the barrier of the intraluminal procedure device and other devices which could be used intraluminally, and of intraluminal transport. The device is introduced over a guide wire to the said situs (Fig. 1).

[0029] A means for withdrawing the procedure device capsule (15) partially to allow for full expansion of the intraluminal procedure device is to have the distal end of the procedure device capsule and the proximal end of the working channel (5) of the intraluminal procedure device threaded together by a screw mechanism (10). Upon rotation of the working channel on the threads of the procedure device capsule, the intraluminal procedure device can be advanced within and out of the procedure device capsule. After completion of work, the intraluminal procedure device can be drawn back into the procedure device capsule and then secured within the capsule by rotating the working channel on the threads of the procedure device capsule in the reverse direction (Fig. 2).

[0030] The intraluminal procedure device functions to aid the performance of intraluminal procedures via endovascular or other intraluminal means and comprises a layer (the "barrier") and a tube (the "working

channel"). The barrier (20) comprises an umbrella-like cone with a generally conical outside surface and a generally conical inside surface (Fig. 2). Materials for fabrication of the cone include flexible, durable, and selectively permeable (such that only certain selected sizes of particles may pass through it) material, for example, polypropylene, polyester, dacron or nylon mesh over supports of stainless steel. The apex of the cone is perforate to allow an exit from the working channel and points downstream in the vasculature. The barrier is suspended over the stainless steel tripod (Fig. 3). Attached circumferentially to the barrier is an expansion device (25, the "Bracer"), such as a balloon (Fig. 4). The balloon can have four to twenty segments, each separated by a diaphragm. Each balloon segment has a separate inflation, deflation channel which allows each segment to have differential inflation directed from a central external control. The external device for inflation and/or deflation of each segment of the Bracer is comprised of means such as syringes or compressed air cylinders in parallel. Each has a valve in series allowing inflation when pressure is applied and passive or active deflation when open. Differential inflation of each balloon segment allows subtle changes in the angle of the working channel in relation to the valve situs. Once inflated the barrier is characterized as capable of allowing blood flow through its permeable surface preventing back pressure and embolization, and providing a working procedure region bounded by the inner surface of the barrier and extending from the barrier's distal ends proximally into the vasculature and heart (Fig. 2).

[0031] The tube of the intraluminal procedure device, the working channel, comprises an elongated flexible cylinder. The working channel is made of durable flexible material, for example, teflon coated polyurethane or other materials which have the following characteristics: flexible, durable, and non-thrombogenic. The tube has a generally cylindrical outside surface and a generally cylindrical inside surface. The proximal open end of the working channel is attached around the barrier's perforated conical apex and its distal end extends out and through the vascular entry point. For use in an adult human, the working channel preferably has an internal diameter of about 0.5 to 10 millimeters making it capable of providing passage for instruments, for example, ultrasound, angiography, debriement, suction, irrigation, retrieval devices, and the tissue cutter, from outside the host to the working procedure region. For use in a host other than an adult human, this internal diameter size range can be varied up or down depending on the size of the host and lumen. It can also be useful to have suction or irrigation applied to the working channel.

[0032] The tissue cutter comprises at least one proximal blade and a cable. The proximal blade (45) comprises a collapsible hinged (30) blade of length varying from about 1.0 to 20 millimeters with sharp cutting surfaces. This range of blade length can vary up or down

depending on the size of host and lumen. Alternatively, the proximal blade can comprise a flexible wire capable of high speed rotation which would deliver a cutting contact to the tissue. The blade is made of rigid durable material, for example, stainless steel or elgiloy. The proximal blade is characterized as capable of passage through the working channel to the working procedure region in an unextended state, and then of extension of itself to allow for cutting of any undesired tissue and finally of return to its unextended state. Additional blades can be attached to the proximal blade to increase the cutting ability of the tissue cutter (Figs. 5,6). For example, two shorter approximately 0.5 to 5.0 millimeter distal blades (40) can be attached through melding, hinging, or other connecting methods, to the distal ends of the proximal blade. This blade length range can vary up or down in size depending on the size of host and lumen. These blades provide sharp cutting surfaces at a range from about thirty to one hundred and fifty degree angles to the proximal blade which allows for simultaneous cutting at various angles.

[0033] The cable (35) of the tissue cutter comprises a flexible durable elongated wire and is characterized as being capable of powering the tissue cutter (Fig. 6). The cable is attached to the proximal blade at a central or off-center position and connected distally to an external motor. For example, the cable can be a steel coaxial cable connected to a DC motor for variable speed rotation.

[0034] The valve introducer device comprises an introducer capsule tube, a pusher device and a bracer. The introducer capsules comprises a cylindrical sleeve having a generally cylindrical outside surface and a generally cylindrical inside surface reinforced at the proximal end which is open, and having a semi-closed distal end with a perforate opening, the distal opening, having a diameter approximately the same as the internal diameter of the introducer channel (50) (Fig. 7). The introducer capsule is made of durable, non-thrombogenic, flexible material, for example, teflon coated polyurethane with a grid or mesh design. The introducer capsule is characterized as being capable of containing and maintaining the prosthetic valve device in its compressed state allowing for easy transport through the host's vasculature. The introducer capsule is reinforced at its base with a solid rather than mesh or grid, for example, solid polyurethane coated with teflon to support the mounting ring and the mounting pins of the prosthetic valve device in its compressed state while within the introducer capsule.

[0035] The bracer (70) is circumferentially attached to the external surface of the introducer capsule at the capsule's proximal end. The bracer comprises a differentially expandable device, such as a series of segmented balloons, and is characterized as having the capability of expanding to hold the introducer capsule in a precise position during delivery of the prosthetic valve device (Fig. 8). Each segmented balloon can have an

inflation/deflation channel to provide autonomous segmental expansion and compression. Differential expansion of the series of segmented balloons is directed from a central external control as done with the intraluminal procedure devices. Inflation of each differentially

[0036] The tube of the valve introducer device, the introducer channel, comprises an elongated flexible cylinder. The introducer channel (50) is made of durable, flexible material, for example, teflon coated polyurethane or other materials which have the following characteristics: flexible, durable, and non-thrombogenic. The introducer channel has a generally cylindrical outside surface and a generally cylindrical inside surface. The proximal end of the introducer channel is attached circumferentially around the distal opening of the introducer capsule and the introducer channel's distal end exits through the vascular entry point (Fig. 9). For use in an adult human, the introducer channel preferably has an internal diameter of about 0.5-10 mm, making it capable of containing the pusher channel (55) of the pusher device. For use in a host other than an adult human, this internal diameter size range can be varied up or down depending on the size of the host and lumen. The introducer channel and pusher channel are also characterized as being capable of allowing suction or irrigation instruments within its lumen.

[0037] The pusher device comprises a disc and a tube. The pusher disc (60) of the pusher device comprises a generally circular disc, with a generally flat distal surface, a generally flat proximal surface and a central opening. The diameter of the opening should be smaller than the diameter used in the introducer channel. The pusher disc is made of a durable, flexible material such as teflon coated polyurethane or other materials which have the following characteristics: flexible and durable. The proximal surface of the pusher disc abuts the prosthetic valve device contained within the introducer capsule (Fig. 9).

[0038] Attached at the pusher disc's distal surface circumferentially around the central opening of the pusher disc is the proximal end of the tube, the pusher channel. The pusher channel, comprises an elongated flexible cylinder and is made of durable, flexible, non-thrombogenic material, that can maintain its structural integrity such that it will not distort upon application of external pressure (e.g. teflon coated polyurethane). The pusher channel has a generally cylindrical outside surface and a generally cylindrical inside surface and has a smaller internal diameter than that used in the introducer channel (Fig. 10). It is characterized as capable of being contained within the lumen of the introducer channel with its distal end extending beyond the vascular entry point via the introducer channel and of allowing passage of the mounting balloon (75) and guide wire (65). It is also characterized as being capable of advancing within the lumen of the introducer channel, upon application of

external pressure at the vascular entry point to advance the pusher disc within the introducer capsule. The pusher channel is also characterized as being capable of allowing suction or irrigation instruments within its lumen.

[0039] The prosthetic valve device comprises a sleeve (80), a valve and an annulus. The sleeve is a flexible cylindrical shaped cylinder having a generally cylindrical outside surface and a generally cylindrical inside surface. The sleeve is secured on its inside surface to the valve and on the base of its outside surface to a compressible annulus, the mounting ring (85) (Figs. 11, 12). Securing means can include chemical bonding, laser welding, stapling, or other means. Securing materials can include polypropylene, polyester, nylon, stainless steel or other inert, durable materials. The sleeve is of durable, host compatible, non-thrombogenic, flexible and compressible material, for example, dacron or polytetrafluorethylene, to allow it to be easily compressed, maneuvered and transported through the vasculature to permit endovascular placement. The sleeve's durability permits secure attachment to other objects and layers, and allows the sleeve to remain intact despite the replacement procedure, and the long term of the prosthetic device within the host. All components of the prosthetic valve device, the mounting ring, sleeve and valve, are flexible, compressible, non-thrombogenic and durable.

[0040] Secured to the inner layer of the prosthetic valve device comprises a valve which functions to permit unidirectional circulatory flow of blood. The valve comprises a cylindrical shaped annulus (100) having a generally cylindrical outside surface and a generally cylindrical inside surface containing at least one cusp (95) to permit blood flow in a single direction. The cusp(s) are attached at the distal end (relative to blood flow) of the cylindrical annulus. The cusp(s) open distally to permit the circulation's flow of blood through the valve situs, and then alternately close centrally to prevent circulation back-flow. The valve is flexible, compressible, host-compatible, and non-thrombogenic. The valve can be, for example, a glutaraldehyde fixed porcine aortic valve which has three cusps that open distally to permit unidirectional blood flow. The valve can also be fresh, cryopreserved or glutaraldehyde fixed allografts or xenografts. The optimal material will be synthetic such that it is manufactured from non-biological materials, non-thrombogenic, flexible such that it can be transported through the vasculature, biocompatible and very durable such that it can withstand a permanent fixation at the valve site. It is highly desirable to use flexible material where the valve is to be inserted via endovascular means.

[0041] The mounting ring (85) of the prosthetic valve device is preferably attached at the base of the outside surface of the sleeve. The mounting ring is made of materials that are durable, have high tensile strength, excellent fatigue characteristics and corrosion resistant

(for example, stainless steel, MP35N or elgiloy) and is structured in a compressible architecture such that it can contract upon application and expand upon release of external pressure and still maintain its basic formation. The mounting ring has a generally cylindrical outside surface and a generally cylindrical inside surface comprised of a series of mounting pins (90) to fix the prosthetic valve device at the designated valve situs (Figs. 13-15). The mounting ring provides endovascular sutureless fixation of the device allowing it to operate autonomously. The pins are secured by melding, welding or other connecting methods, at about 30 to about 150 degree angles to the mounting ring. The composite of angles provides for secure fixation such that the prosthetic valve device can tolerate the degree and directional pressure variations on the valve occurring during the different phases of the cardiac cycle. As uniform pressure is exerted at the inner surface of the mounting ring, as for example by inflation of the mounting balloon, the mounting ring expands and the pins extend into and secure to the lumen wall.

[0042] Once the endovascular implantation of the prosthetic valve device is completed in the host, the function of the prosthetic valve device can be monitored by the same methods as used to monitor valve replacements done by open heart surgery. Routine physical examination, periodic echocardiography or angiography can be performed. In contrast to open heart surgery, however, the host requires a short recovery period and can return home within one day of the endovascular procedure. The prosthetic valve device can be used in any patient where bioprosthetic valves are indicated, namely elderly patients with cardiac valve diseases, and patients unable to tolerate open heart procedures or life-long anticoagulation. In addition, with the development of longer-life, flexible, non-thrombogenic synthetic valve alternatives to bioprostheses, the prosthetic valve device will be indicated in all patients where the relative advantages of the life-span, the non-thrombogenic quality, and the ease of insertion of prosthetic valve devices outweigh the disadvantages of mechanical valves. Anticoagulation may be beneficial in certain clinical situations for either short or long term use.

[0043] The intraluminal procedure device, the procedure device capsule and the tissue cutter can be independently applied, or applied in conjunction with each other, to instrumentation at or removal of cardiac, aortic, cerebrovascular, mesenteric, renal, or peripheral vessel valves or tissue, and would be especially important anywhere in the cardiac or vascular system where peripheral embolization is problematic or accurate positioning of instruments is essential. They can also be used in other body lumens, for example, the gastrointestinal, genitourinary, biliary, and respiratory tracts. In addition, the valve replacement system can be used to supplant as well as replace a host's valve or prosthesis. In that procedure the dysfunctional valve or prosthesis is not removed by the tissue cutter, and the prosthetic valve

device is fixated at a vascular situs such that the device supplants the function of the dysfunctional valve or prosthesis. Also, the devices could be used in non-human species, for example, other mammals.

## Claims

1. A device for performing an intraluminal procedure at a situs in a patient, which has a barrier (20) to about the lumen wall when in an expanded condition; the device including a capsule having a tubular flexible sleeve (15) with a generally cylindrical outside surface and a generally cylindrical inside surface, the capsule being capable of transporting the barrier (20) endoluminally to said situs, the barrier (20) being movable relative to the sleeve (15) to exit from the sleeve, and being expandable to about the lumen wall when so exited to encircle the situs, characterized in that the barrier (20) has a circumferentially differentially expandable bracer (25) to allow changes in the angle of a working channel (5) of the barrier, in relation to the situs.

2. The device of claim 1, wherein the barrier (20) is of selectively permeable material.

3. The device of claim 1, further comprising:

a tissue cutter for removal of undesired tissue, the tissue cutter having at least one blade (45) and a cable (35), said at least one blade (45) being movable to an unextended condition and being capable of endovascular passage to the encircled situs while in the unextended condition.

4. The device of claim 4, wherein:

said at least one blade (45) has a hinge (30) for allowing movement of the blade (45) to and from unextended and extended conditions.

5. A device for performing an intraluminal procedure at a situs in a patient, which has a valve introducer for delivering a replacement valve (80), the valve introducer having an introducer capsule, an introducer channel (50) and a pusher (60), the introducer capsule being configured to retain the replacement valve (80) and endovascularly deliver the replacement valve to said situs, the introducer channel (50) having an end attached to the introducer capsule, the replacement valve being delivered by being forced from the introducer capsule,

characterized by a bracer (70) attached to the introducer capsule and expandable to hold the introducer capsule in position during delivery of the replacement valve.

6. The device of claim 5, wherein said bracer (70) is circumferentially differentially expansible so as to have the capability of holding said introducer capsule accurately in position during delivery of the replacement valve device (80).

7. The device of claim 5, wherein said pusher (60) is a disc.

#### Patentansprüche

1. Vorrichtung zur Durchführung eines intraluminalen Eingriffs an einer Stelle in einem Patienten, die eine Barriere (20) aufweist, die an der Lumenwand anliegt, wenn sie sich in einem ausgedehnten Zustand befindet; wobei die Vorrichtung eine Kapsel mit einer röhrenförmigen flexiblen Hülse (15) mit einer allgemein zylindrischen Außenfläche und einer allgemein zylindrischen Innenfläche aufweist, wobei die Kapsel fähig ist, die Barriere (20) endoluminal an die Stelle zu transportieren, wobei die Barriere (20) in bezug auf die Hülse (15) so bewegt werden kann, daß sie aus der Hülse austritt, und ausgedehnt werden kann, so daß sie an der Lumenwand anliegt, wenn sie so ausgetreten ist, um die Stelle zu umfassen, dadurch gekennzeichnet, daß die Barriere (20) einen Umfang entlang differenziert erweiterbare Verspreizung (25) aufweist, um Änderungen im Winkel eines Arbeitskanals (5) der Barriere in bezug auf die Stelle zu ermöglichen.

2. Vorrichtung nach Anspruch 1, worin die Barriere (20) aus selektiv durchlässigem Material besteht.

3. Vorrichtung nach Anspruch 1, weiters umfassend:

eine Gewebeschnideeinrichtung zum Entfernen von unerwünschtem Gewebe, wobei die Gewebeschnideeinrichtung zumindest eine Klinge (45) und ein Kabel (35) aufweist, wobei die zumindest eine Klinge (45) in einen unausgefahrenen Zustand bewegt werden kann und zum endovaskulären Durchtritt zur umfaßten Stelle fähig ist, während sie sich im unausgefahrenen Zustand befindet.

4. Vorrichtung nach Anspruch 3, worin:

die zumindest eine Klinge (45) ein Gelenk (30) aufweist, um es zu ermöglichen, die Klinge (45) aus dem unausgefahrenen in den ausgefahrenen Zustand und zurück zu bewegen.

5. Vorrichtung zur Durchführung eines intraluminalen Eingriffs an einer Stelle in einem Patienten, die eine Ventil-Einsatzvorrichtung zum Anbringen eines Ersatzventils (80) aufweist, wobei die Ventil-Ein-

setzvorrichtung eine Einsatzkapsel, einen Einsatzkanal (50) und einen Schieber (60) aufweist, wobei die Einsatzkapsel eine solche Konfiguration aufweist, daß sie das Ersatzventil (80) hält und es endovaskulär an die Stelle hinbringt, wobei ein Ende des Einsatzkanals (50) an der Einsatzkapsel befestigt ist, wobei das Ersatzventil dadurch angebracht wird, daß es aus der Einsatzkapsel herausgedrängt wird, dadurch gekennzeichnet, daß eine Verspreizung (70) an der Einsatzkapsel befestigt und so erweiterbar ist, daß sie die Einsatzkapsel während des Anbringens des Ersatzventils in Position hält.

6. Vorrichtung nach Anspruch 5, worin die Verspreizung (70) den Umfang entlang differenziert erweiterbar ist, so daß sie die Fähigkeit aufweist, die Einsatzkapsel während des Anbringens der Ersatzventilvorrichtung (80) präzise in Position zu halten.

7. Vorrichtung nach Anspruch 5, worin der Schieber (60) eine Scheibe ist.

#### Revendications

1. Dispositif pour exécuter des procédés intraluminaux à un site dans un patient, qui a une barrière (20) pour buter contre la paroi de lumière lorsqu'il est dans un état expansé; le dispositif incluant une capsule avec un manchon flexible tubulaire (15) avec une surface extérieure généralement cylindrique et une surface intérieure généralement cylindrique, la capsule étant apte à transporter la barrière (20) à l'intérieur de la lumière audit site, la barrière (20) étant déplaçable par rapport au manchon (15) pour sortir du manchon et étant expansible pour buter contre la paroi de lumière lorsqu'elle est ainsi sollicitée pour encercler le site, caractérisé en ce que la barrière (20) a des bras (25) expansibles circonférentiellement différentiellement pour permettre des changements de l'angle d'un canal de travail (5) de la barrière, relativement au site.

2. Dispositif selon la revendication 1, où la barrière (20) est en matériau sélectivement perméable.

3. Dispositif selon la revendication 1 comprenant en outre :

un organe de coupe de tissu pour retirer du tissu non voulu, l'organe de coupe de tissu comportant au moins une lame (45) et un câble (35), ladite au moins une lame (45) étant déplaçable à un état non étendu et étant apte à passer d'une manière endovasculaire au site encerclé en se trouvant dans l'état non étendu.



4. Dispositif selon la revendication 4, où :

ladite au moins une lame (45) a une articulation (30) pour permettre le déplacement de la lame (45) vers et au loin des états non étendu et étendu.

5. Dispositif pour exécuter un procédé intraluminal à un site dans un patient, qui comporte un organe d'introduction de vanne pour transmettre une vanne de remplacement (80), l'organe d'introduction de vanne comportant une capsule d'organe d'introduction, un canal d'organe d'introduction (50) et un poussoir (60), la capsule de l'organe d'introduction étant configurée pour retenir la vanne de remplacement (80) et pour transmettre d'une manière endovasculaire la vanne de remplacement audit site, le canal d'introduction (50) ayant une extrémité fixée à la capsule de l'organe d'introduction, la vanne de remplacement étant transmise en étant forcée au loin de la capsule de l'organe d'introduction, caractérisé par un bracon (70) fixé à la capsule de l'organe d'introduction et expansible pour tenir la capsule de l'organe d'introduction en position pendant la transmission de la vanne de remplacement.
6. Dispositif selon la revendication 5, où ledit bracon (70) est expansible circonférentiellement différemment de façon à être apte à tenir ladite capsule de l'organe d'introduction d'une manière précise en position pendant la transmission du dispositif de vanne de remplacement (80).
7. Dispositif selon la revendication 5, où ledit poussoir (60) est un disque.

40

45

50

55

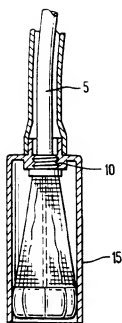


FIG. 1

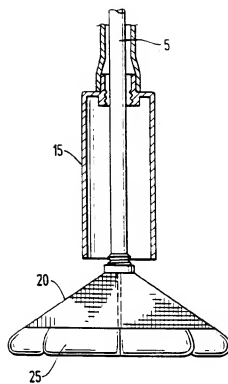


FIG. 2




FIG. 4




FIG. 3




FIG. 5




FIG. 6

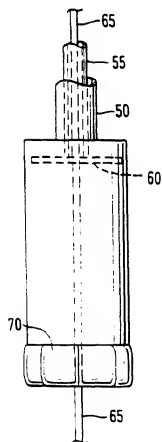


FIG. 7

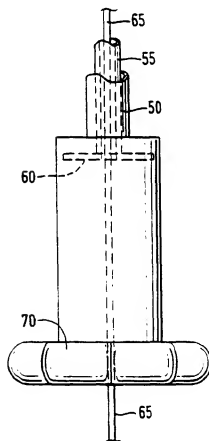


FIG. 8

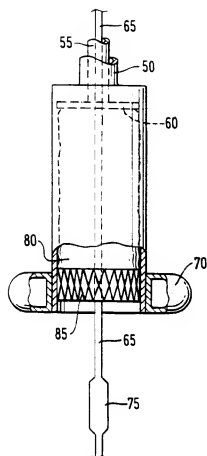


FIG. 9

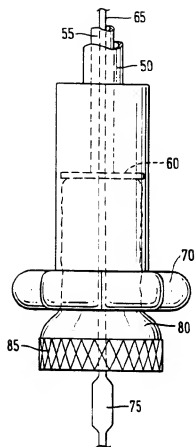


FIG. 10




FIG. 11




FIG. 12




FIG. 13a



FIG. 13b




FIG. 14a



FIG. 14b




FIG. 15a




FIG. 15b